



Summary of the CovaWound™ survey

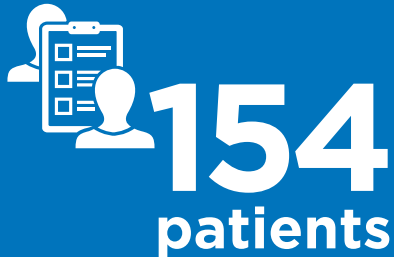


Setting

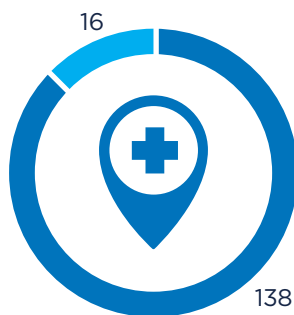


Hospital	138
Wound Care Clinics	16

User type

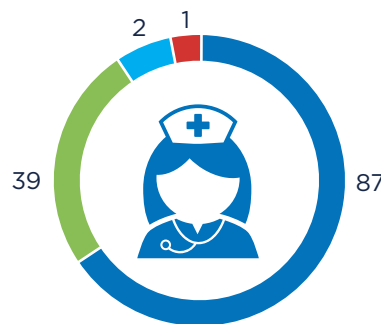

Hospital Nurse	87
District Nurse	2
Tissue Viability Nurse	39
Research Nurse	1

Wound aetiology

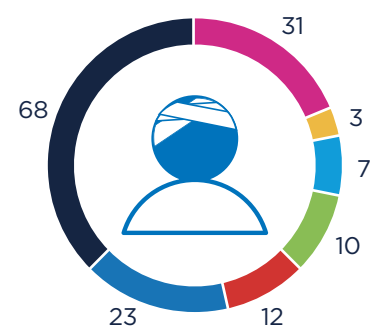


Burns	23
Cavity wounds	7
Diabetic foot ulcers	10
Leg ulcers	12
Pressure ulcers	31
Surgical wounds	3
Wound type unrecorded	68

Dressing type




143

CovaWound™
Silicone Foam



CovaWound™
Silicone Foam (Bordered)



CovaWound™
Hydrocolloid

11




CovaWound™
Hydrocolloid (Bordered)

76% of Clinical Users rated **CovaWound™** as **good** or **very good** compared to their usual dressing.



32% of Clinical Users rated **CovaWound™** as **excellent** compared to their usual dressing.


Comparisons



of Patients, when rating **overall comfort**, rated **Covawound™** as the **same** or **better** than their comparison dressing.



of Patients, when rating **pain levels on dressing removal**, rated **CovaWound™** as the **same** or **better** than their comparison dressing.



of Clinicians, when rating **ease of dressing removal**, rated **CovaWound™** as the **same** or **better** than their comparison dressing.



of Clinicians, when rating **condition of the surrounding skin**, rated **CovaWound™** as the **same** or **better** than their comparison dressing.

Brands Compared

- ALLEVYN Gentle
- Mepilex®
- KerraFoam®
- Biatain® Silicone
- Aquacel® Foam
- DuoDERM®

